



## Mounting adapter MNT-113

### Accessory

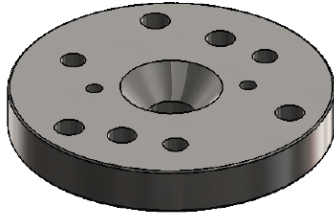

| TAG | X LOC | Y LOC | SIZE                                                         |
|-----|-------|-------|--------------------------------------------------------------|
| A1  | -0.95 | 0.21  | <MOD-DIAM> 0.14 THRU ALL<br>8-32 UNC THRU ALL                |
| A2  | -0.06 | -0.31 |                                                              |
| A3  | -0.06 | 0.72  |                                                              |
| B1  | -0.75 | -0.36 | <MOD-DIAM> 0.16 THRU ALL<br>10-32 UNF THRU ALL               |
| B2  | -0.65 | 0.83  |                                                              |
| B3  | -0.36 | -0.36 |                                                              |
| B4  | -0.36 | 0.77  |                                                              |
| B5  | 0.33  | 0.15  |                                                              |
| C1  | -0.71 | 0.41  | <MOD-DIAM> 0.09 THRU ALL<br>4-40 UNC THRU ALL                |
| C2  | 0.00  | 0.00  |                                                              |
| D1  | -0.36 | 0.21  | <MOD-DIAM> 0.26 THRU ALL<br><HOLE-SINK><MOD-DIAM> 0.55 X 82° |

All dimensions are in inches.

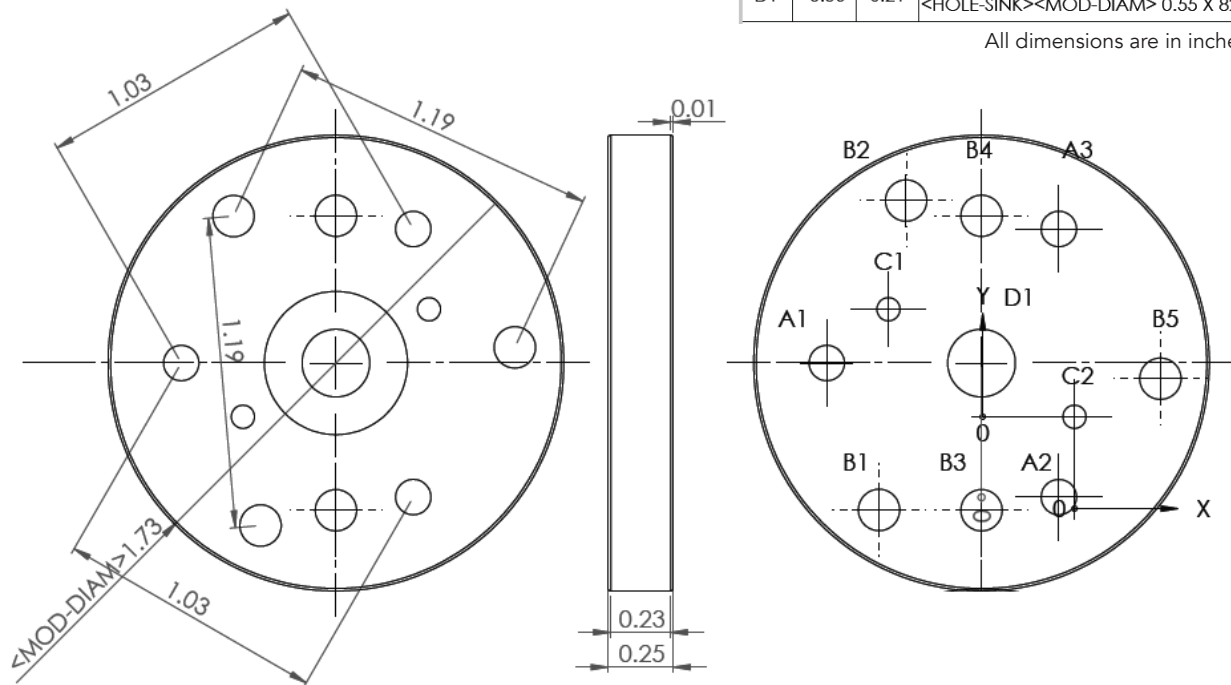

### Description

Universal accelerometer mounting adaptor, for use with 28959G portable vibration calibrator.



Continued product improvement necessitates that Endevco reserve the right to modify these specifications without notice. Endevco maintains a program of constant surveillance over all products to ensure a high level of reliability. This program includes attention to reliability factors during product design, the support of stringent Quality Control requirements, and compulsory corrective action procedures. These measures, together with conservative specifications have made the name Endevco synonymous with reliability. 090119